

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

APR 06 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130290</u> ✓	
Name <u>Derek Sitz</u>		ID# <u>4092</u>	Date <u>3-28-10</u> ✓
A	Agency <u>Anchorage Police Dept.</u>		Phone # <u>786 8900</u>
Instrument Location <u>Anchorage Jail</u> ✓			
Alco S/N <u>B72446</u> ✓		Target Value <u>.078</u> ✓	High Pressure <u>250</u>
B	Alco Test Values		
	<u>.071</u> 1 <sup>st</sup> Alco	<u>.076</u> 2 <sup>nd</sup> Alco	✓
Signature <u>Derek Sitz</u> ✓			
(OVER)			

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
Nita J. Bolz

Scientific Director



State Breath Alcohol Program

Subscribed and sworn before me this 26<sup>th</sup> day of April, 2010.

Carolyn M. Noland  
Carolyn M. Noland

Notary Public, State of Alaska

Commission Expires with Office

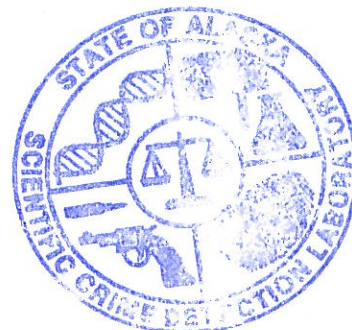

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130290 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

T

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130293

MARCH 26, 2010 ✓

OPERATOR'S NAME:

SITZ, DEREK W

OPERATOR'S NUMBER: 4056

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 1234567

DEPT/AGENCY: ANCI

CASE/REPORT: 00-1234

TEST TYPE: V

ALCO TARGET VALUE: .078 ✓

ALCO S/N: B72446 ✓

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 29.25 in ✓

ALCO TARGET	.076	23:38
BLANK TEST	.000	23:39
INTERNAL STANDARD	VERIFIED	23:39
ALCO TV 29.25 in	.071 ✓	23:39
BLANK TEST	.000	23:40
SUBJECT SAMPLE	.000	23:41
BLANK TEST	.000	23:41
ALCO TV 29.25 in	.076 ✓	23:42
BLANK TEST	.000	23:43

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130293 ✓

MARCH 26, 2010 ✓

TIME 23:44

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 48c

BREATH TUBE: 41c

BAROMETER: 29.25 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~